



Selection guide for
CAMLOG® Healing caps and
impression posts

Emergence profile is congruent in shape

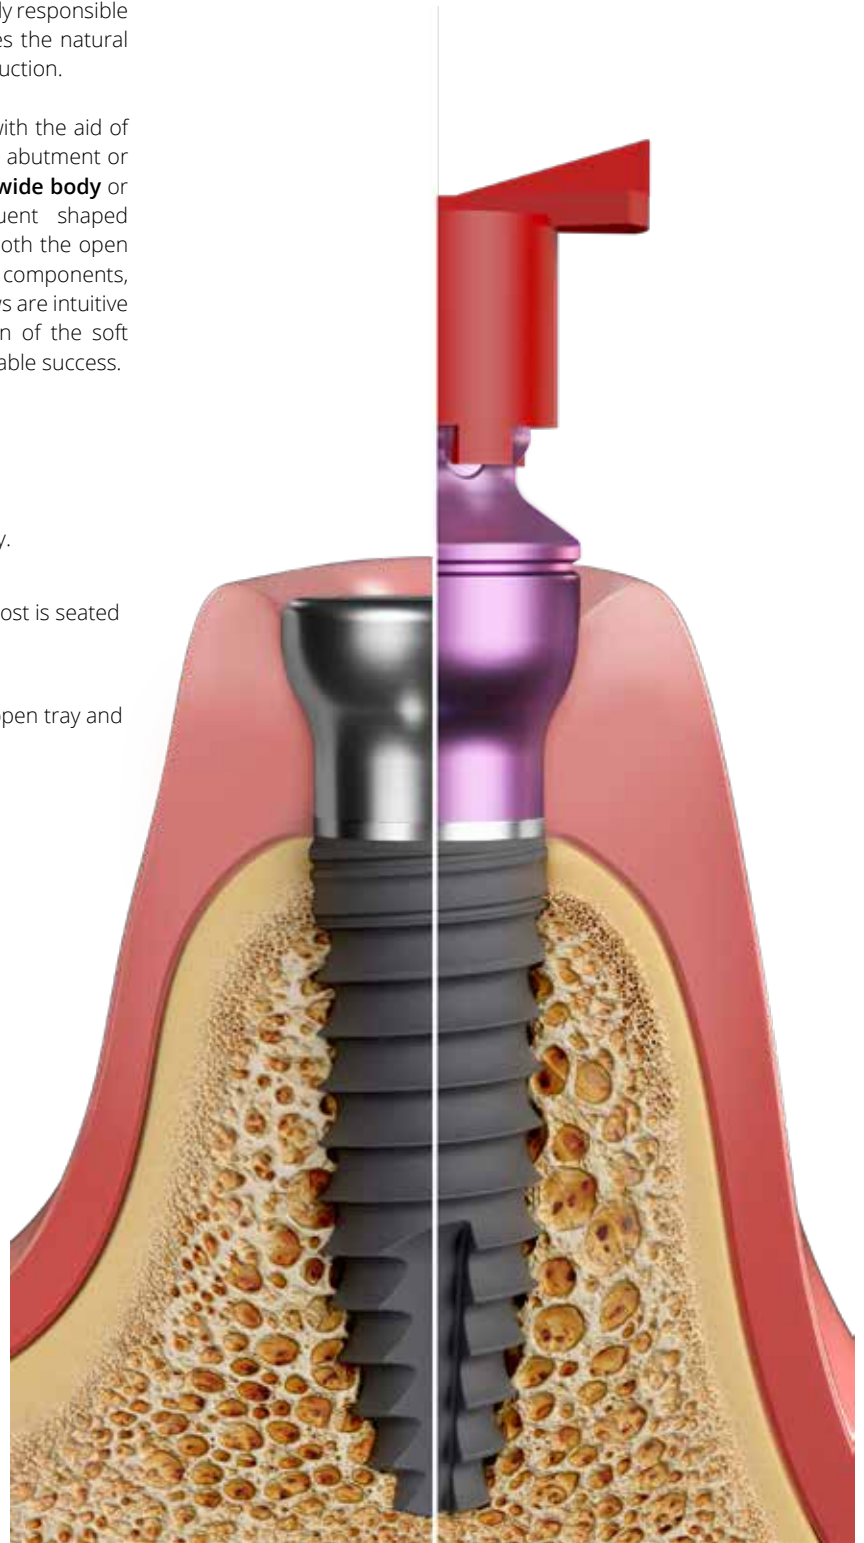
For CAMLOG® Healing caps and impression posts

A stable soft tissue cuff is crucial for the success of implant therapy in several respects. Not only is a healthy gingiva predominantly responsible for the preservation of the marginal bone, it also ensures the natural and optimized red-white esthetics of the implant reconstruction.

The soft tissue can be optimally shaped or conditioned with the aid of CAMLOG® Healing caps. Depending on the intended final abutment or type of soft tissue shaping with healing caps **cylindrical, wide body** or **wide body narrow**, impression posts with congruent shaped emergence profiles are available. These are offered for both the open and closed tray techniques. Due to the congruent shaped components, a collapse of the soft tissue cuff is prevented. The workflows are intuitive yet flexible - the best possible standardized preparation of the soft tissue for receiving an implant crown and for long-term stable success.


Additional product features at a glance

- **Sterile delivery**
Direct insertion in the mouth - no preparation necessary.
- **Screw safeguard**
The screw can only be tightened when the impression post is seated correctly.
- **Screw retention**
The fixing screw is secured from falling out in both the open tray and closed tray impression posts.




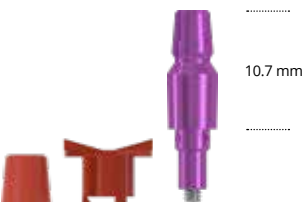

Product details healing caps and impression posts

Standard: cylindrical


	Article	Art. No.	Ø	GH	G Ø
	CAMLOG® Healing caps, cylindrical sterile Material Titanium alloy	J2015.3320	3.3 mm	2.0 mm	3.5 mm
		J2015.3340		4.0 mm	3.5 mm
		J2015.3360		6.0 mm	3.5 mm
		J2015.3820	3.8 mm	2.0 mm	4.0 mm
		J2015.3840		4.0 mm	4.0 mm
		J2015.3860*		6.0 mm	4.0 mm
		J2015.4320	4.3 mm	2.0 mm	4.5 mm
		J2015.4340		4.0 mm	4.5 mm
		J2015.4360*		6.0 mm	4.5 mm
		J2015.5020	5.0 mm	2.0 mm	5.2 mm
		J2015.5040		4.0 mm	5.2 mm
		J2015.5060*		6.0 mm	5.2 mm
		J2015.6020	6.0 mm	2.0 mm	6.2 mm
		J2015.6040		4.0 mm	6.2 mm
J2015.6060*	6.0 mm	6.2 mm			


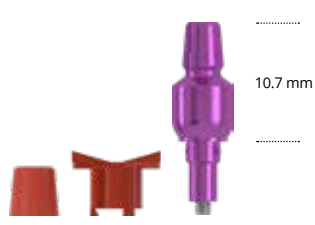

* Suitable for bite registration

Healing caps are for single use only and must not be resterilized.


	Article	Art. No.	Ø
	CAMLOG® Impression post, open tray, cylindrical incl. fixing screw (the fixing screw can be shortened extra-orally by 3 mm with a screwdriver, hex), sterile Material Titanium alloy	K2125.3300	3.3 mm
		K2125.3800	3.8 mm
		K2125.4300	4.3 mm
		K2125.5000	5.0 mm
		K2125.6000	6.0 mm
	CAMLOG® Impression post, closed tray, cylindrical incl. impression cap, bite registration cap and fixing screw, sterile Material Titanium alloy/PBT	K2115.3300	3.3 mm
		K2115.3800	3.8 mm
		K2115.4300	4.3 mm
		K2115.5000	5.0 mm
		K2115.6000	6.0 mm
	Impression cap for impression post, closed tray (6 units) Material PBT	J2111.3310	3.3 mm
		J2111.3810	3.8 mm
		J2111.4310	4.3 mm
		J2111.5010	5.0 mm
		J2111.6010	6.0 mm




Standard: wide body

	Article	Art. No.	Ø	GH	G Ø
	CAMLOG® Healing caps, wide body sterile Material Titanium alloy	J2014.3320	3.3 mm	2.0 mm	4.4 mm
		J2014.3340		4.0 mm	4.5 mm
		J2014.3360		6.0 mm	4.5 mm
		J2014.3820	3.8 mm	2.0 mm	4.9 mm
		J2014.3840		4.0 mm	5.0 mm
		J2014.3860		6.0 mm	5.0 mm
		J2014.4320	4.3 mm	2.0 mm	5.4 mm
		J2014.4340		4.0 mm	5.5 mm
		J2014.4360		6.0 mm	5.5 mm
		J2014.5020	5.0 mm	2.0 mm	6.1 mm
		J2014.5040		4.0 mm	6.2 mm
		J2014.5060		6.0 mm	6.2 mm
		J2014.6020	6.0 mm	2.0 mm	7.1 mm
		J2014.6040		4.0 mm	7.2 mm
		J2014.6060		6.0 mm	7.2 mm

	Article	Art. No.	Ø
	CAMLOG® Impression post, open tray, wide body incl. fixing screw (the fixing screw can be shortened extra-orally by 3 mm with a screwdriver, hex), sterile Material Titanium alloy	K2124.3300	3.3 mm
		K2124.3800	3.8 mm
		K2124.4300	4.3 mm
		K2124.5000	5.0 mm
		K2124.6000	6.0 mm
	CAMLOG® Impression post, closed tray, wide body incl. impression cap, bite registration cap and fixing screw, sterile Material Titanium alloy/PBT	K2114.3300	3.3 mm
		K2114.3800	3.8 mm
		K2114.4300	4.3 mm
		K2114.5000	5.0 mm
		K2114.6000	6.0 mm
	Impression cap for impression post, closed tray (6 units) Material PBT	J2111.3310	3.3 mm
		J2111.3810	3.8 mm
		J2111.4310	4.3 mm
		J2111.5010	5.0 mm
		J2111.6010	6.0 mm



Standard: wide body narrow

	Article	Art. No.	Ø	GH	G Ø
	CAMLOG® Healing caps, wide body narrow sterile Material Titanium alloy	J2024.3340	3.3 mm	4.0 mm	4.5 mm
		J2024.3360		6.0 mm	4.5 mm
		J2024.3840	3.8 mm	4.0 mm	5.0 mm
		J2024.3860		6.0 mm	5.0 mm
		J2024.4340	4.3 mm	4.0 mm	5.5 mm
		J2024.4360		6.0 mm	5.5 mm
		J2024.5040	5.0 mm	4.0 mm	6.2 mm
		J2024.5060		6.0 mm	6.2 mm
		J2024.6040	6.0 mm	4.0 mm	7.2 mm
		J2024.6060		6.0 mm	7.2 mm

	Article	Art. No.	Ø
	CAMLOG® Impression post, open tray, wide body narrow incl. fixing screw (the fixing screw can be shortened extra-orally by 3 mm with a screwdriver, hex), sterile Material Titanium alloy	K2124.3301	3.3 mm
		K2124.3801	3.8 mm
		K2124.4301	4.3 mm
		K2124.5001	5.0 mm
		K2124.6001	6.0 mm
	CAMLOG® Impression post, closed tray, wide body narrow incl. impression cap, bite registration cap and fixing screw, sterile Material Titanium alloy/PBT	K2114.3301	3.3 mm
		K2114.3801	3.8 mm
		K2114.4301	4.3 mm
		K2114.5001	5.0 mm
		K2114.6001	6.0 mm
	Impression cap for impression post, closed tray (6 units) Material PBT	J2111.3310	3.3 mm
		J2111.3810	3.8 mm
		J2111.4310	4.3 mm
		J2111.5010	5.0 mm
		J2111.6010	6.0 mm

Product details healing caps and impression posts




Platform Switching: cylindrical and wide body

	Article	Art. No.	Ø	GH	G Ø
	CAMLOG® Healing cap PS, cylindrical** for Platform Switching, sterile Material Titanium alloy	K2005.3820	3.8 mm	2.0 mm	3.3 mm
		K2005.3840		4.0 mm	3.3 mm
		K2005.3860*		6.0 mm	3.3 mm
		K2005.4320	4.3 mm	2.0 mm	3.8 mm
		K2005.4340		4.0 mm	3.8 mm
		K2005.4360*		6.0 mm	3.8 mm
		K2005.5020	5.0 mm	2.0 mm	4.4 mm
		K2005.5040		4.0 mm	4.4 mm
		K2005.5060*		6.0 mm	4.4 mm
		K2005.6020	6.0 mm	2.0 mm	5.1 mm
		K2005.6040		4.0 mm	5.1 mm
K2005.6060*	6.0 mm	5.1 mm			
	CAMLOG® Healing caps PS, wide body** for Platform Switching, sterile Material Titanium alloy	K2004.3840	3.8 mm	4.0 mm	5.0 mm
		K2004.3860		6.0 mm	5.0 mm
		K2004.4340	4.3 mm	4.0 mm	5.5 mm
		K2004.4360		6.0 mm	5.5 mm
		K2004.5040	5.0 mm	4.0 mm	6.2 mm
		K2004.5060		6.0 mm	6.2 mm
		K2004.6040	6.0 mm	4.0 mm	7.2 mm
		K2004.6060		6.0 mm	7.2 mm

* Suitable for bite registration
















** for CAMLOG® Implants with K article numbers

Healing caps are for single use only and must not be resterilized.

	Article	Art. No.	Ø
	CAMLOG® Impression post PS, open tray, for Platform Switching incl. fixing screw (the fixing screw can be shortened extra-orally by 3 mm with a screwdriver, hex), sterile Material Titanium alloy	K2122.3800	3.8 mm
		K2122.4300	4.3 mm
		K2122.5000	5.0 mm
		K2122.6000	6.0 mm
	CAMLOG® Impression post PS, closed tray, for Platform Switching incl. impression cap, bite registration cap and fixing screw, sterile Material Titanium alloy/PBT	K2111.3800	3.8 mm
		K2111.4300	4.3 mm
		K2111.5000	5.0 mm
		K2111.6000	6.0 mm
	Impression cap for impression post, closed tray (6 units) Material PBT	J2111.3310	3.3 mm
		J2111.3810	3.8 mm
		J2111.4310	4.3 mm
		J2111.5010	5.0 mm
		J2111.6010	6.0 mm

Selection guide

Healing caps and impression posts according to preferred impression technique

	Healing caps	Impression posts, <u>open tray</u>	Impression posts, <u>closed tray</u>		
Standard	cylindrical	 J2015.XXY0	 K2125.XX00	 K2115.XX00	
	wide body	 J2014.XXY0	 K2124.XX00	 K2114.XX00	
	wide body narrow	 J2024.XXY0	 K2124.XX01	 K2114.XX01	
	Platform Switching (PS)	cylindrical	 K2005.XXY0	 K2122.XX00	 K2111.XX00
		wide body	 K2004.XXY0	 K2122.XX00	 K2111.XX00

Headquarters

CAMLOG Biotechnologies GmbH | Margarethenstr. 38 | 4053 Basle | Switzerland
Telephone +41 61 565 41 00 | Fax +41 61 565 41 01 | info@camlog.com | www.biohorizonscamlog.com

CAMLOG Biotechnologies GmbH or BioHorizons Inc. respectively may market products only upon clearance and approval by the respective national authorities.
Therefore, not all products may be available in your country.

CAMLOG® is a registered trademark of CAMLOG Biotechnologies GmbH.

Inspiring excellence in oral reconstruction

